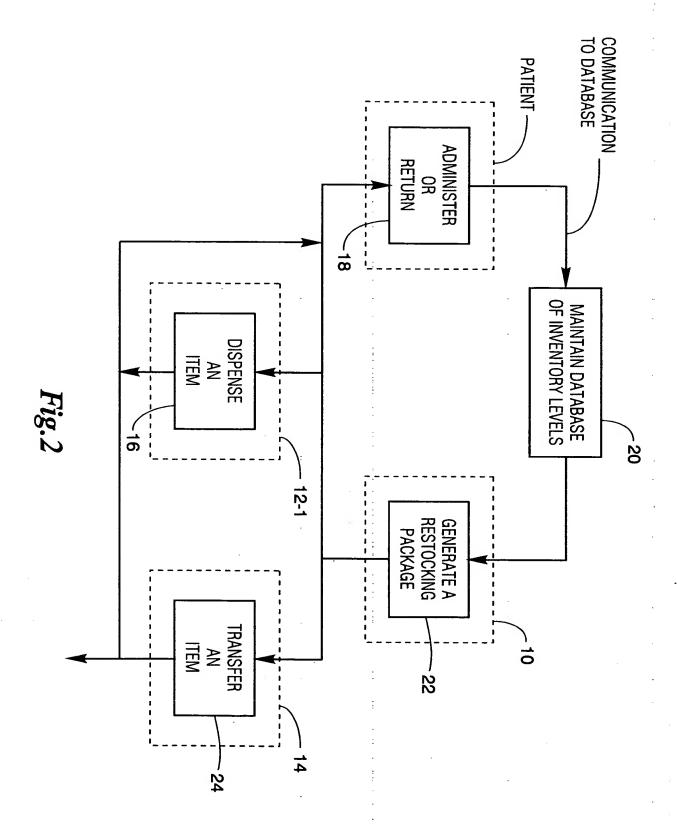
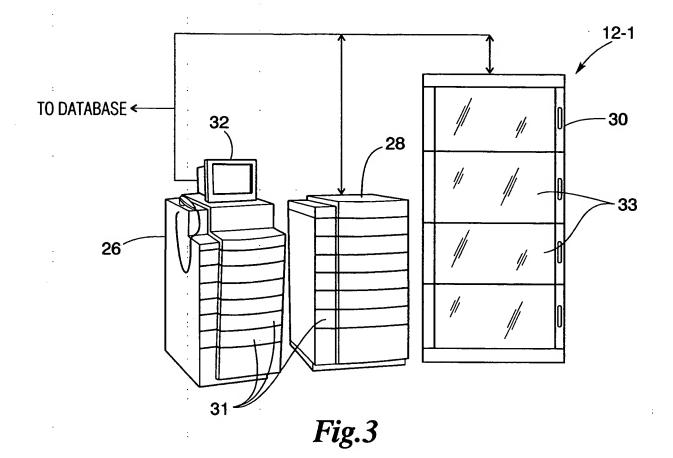
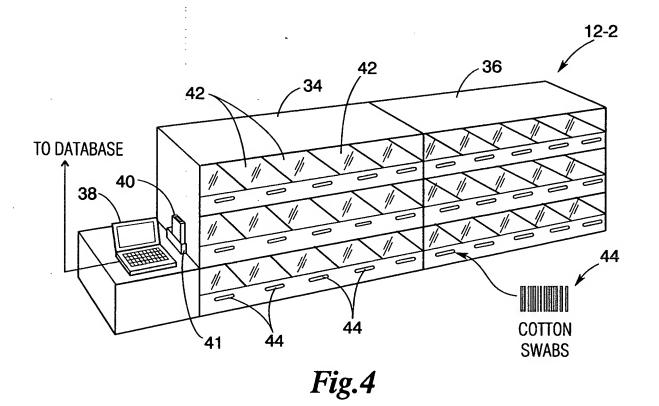
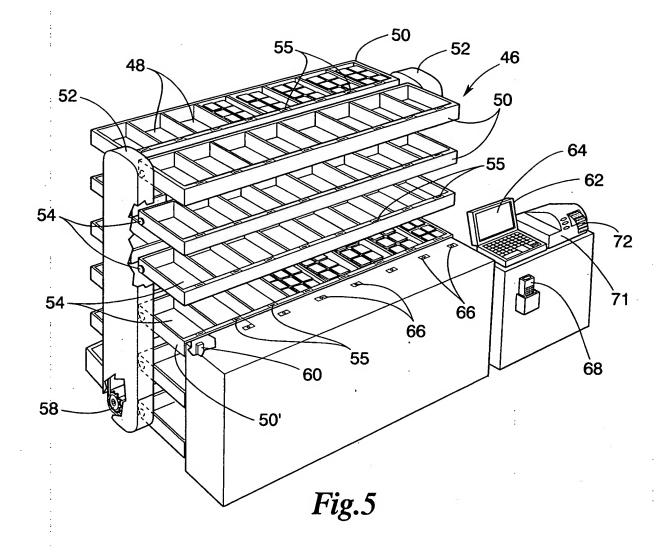



Fig. 1











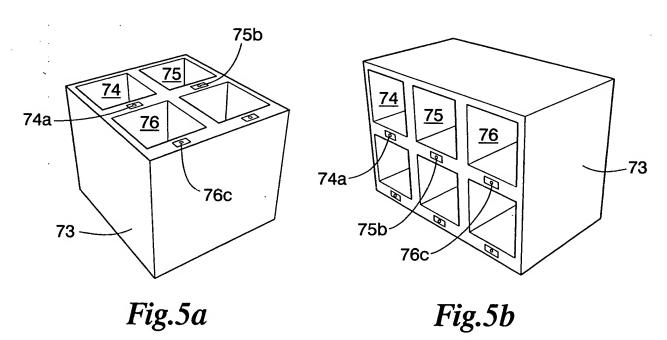

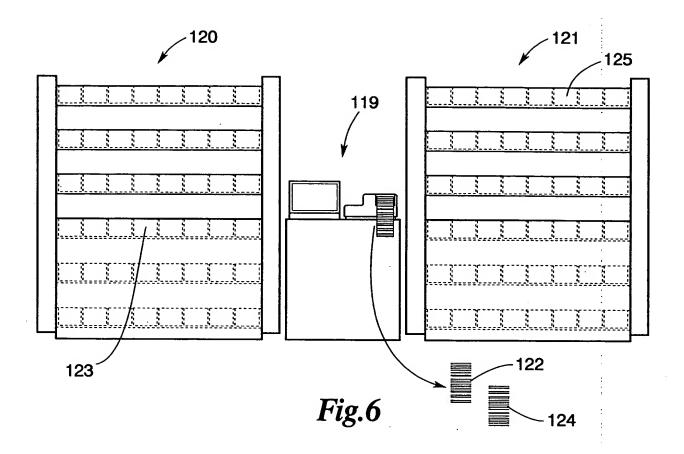

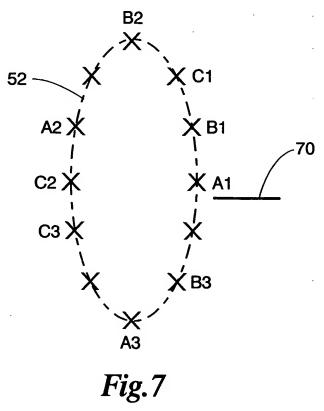

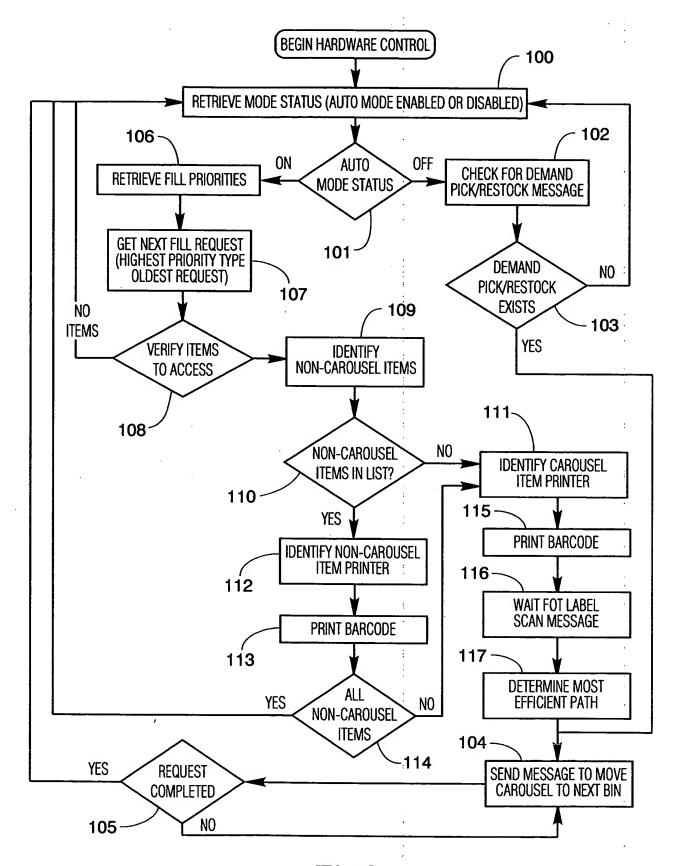


Fig.8

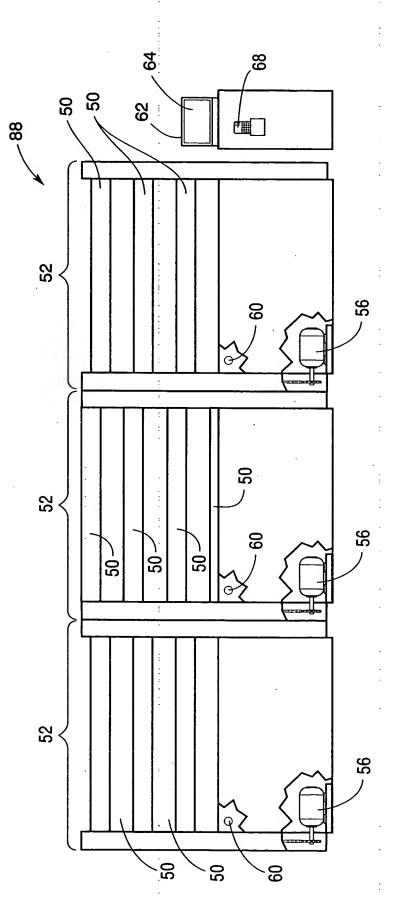
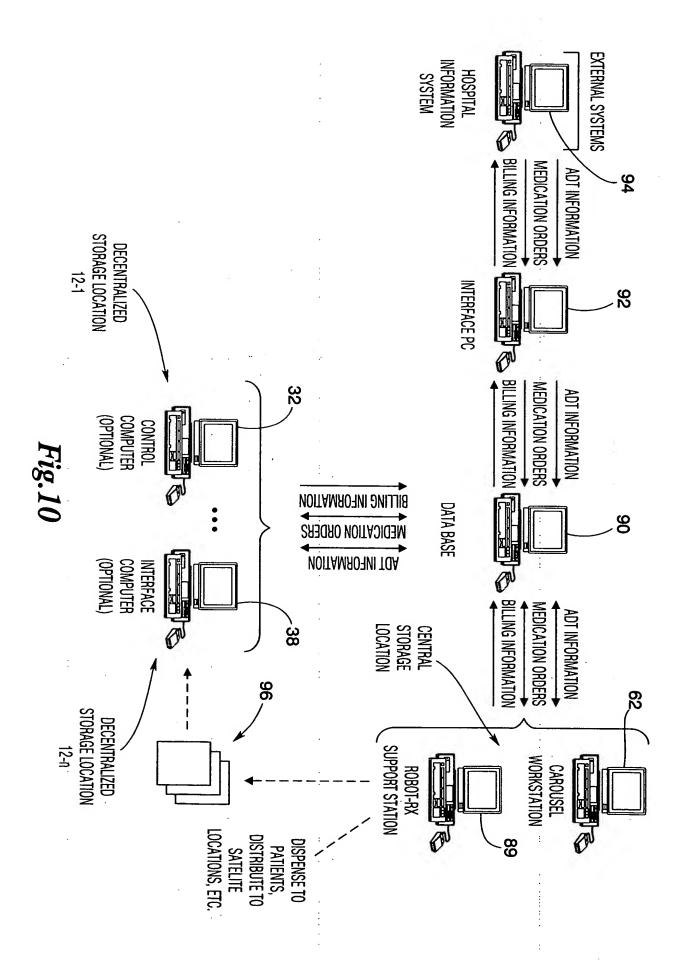


Fig. 9





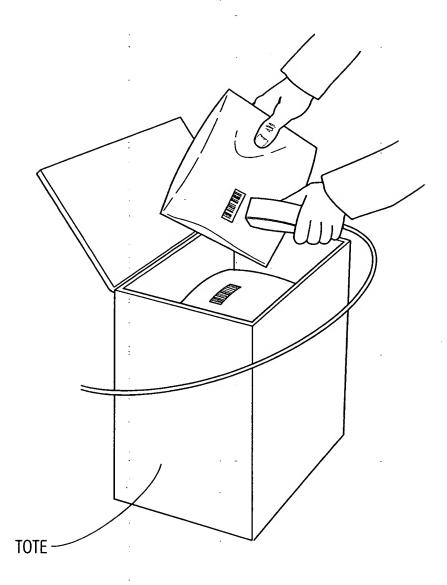



Fig.11

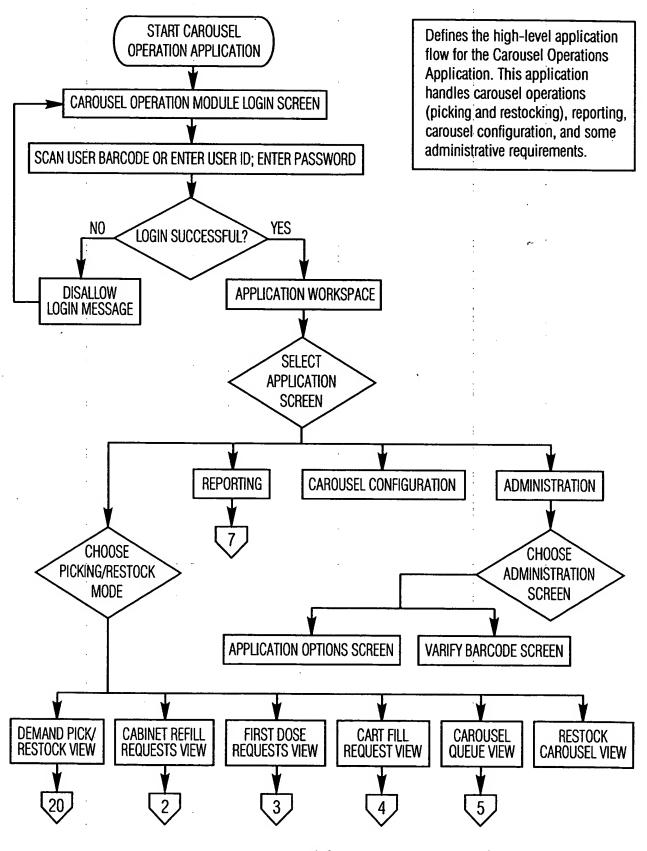


A1

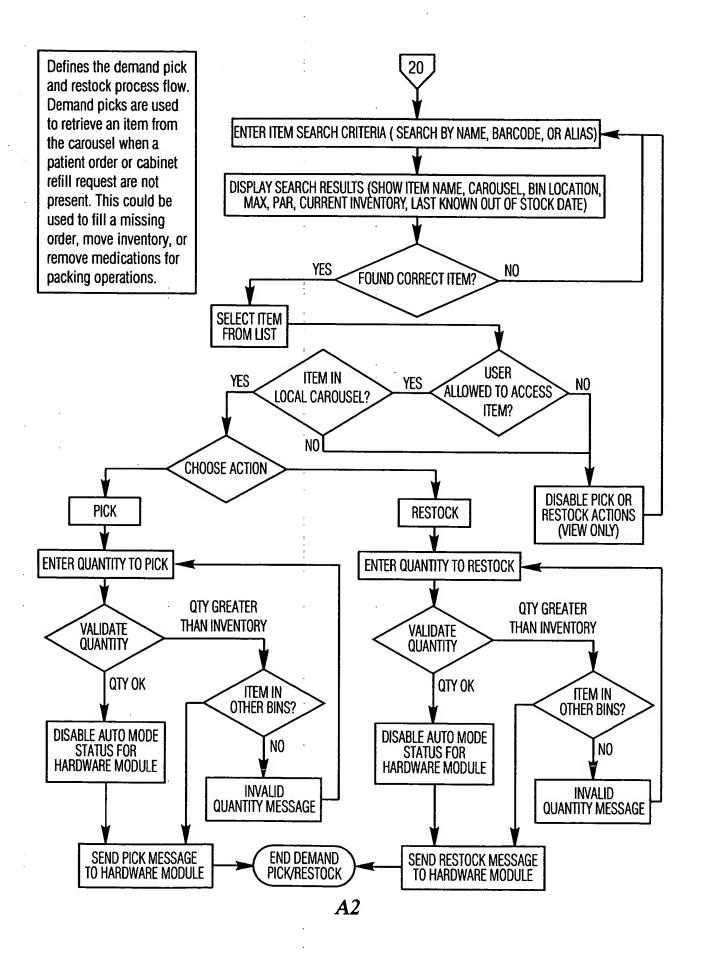


Defines the cabinet refilling process. This allows the viewing of queued cabinet refill requests and the ability to selectively send these requests on a station or individual request level to the carousel.

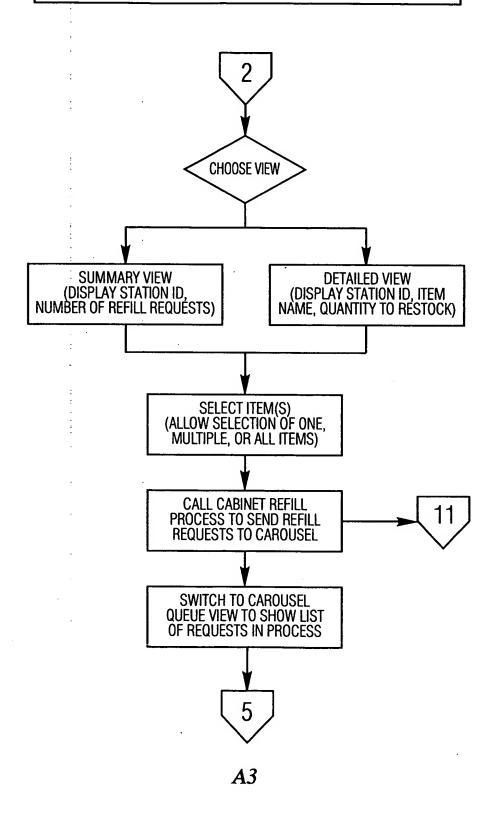


Defines the patient first dose filling process. This allows the viewing of queued first doses and the ability to selectively send these requests on a patient or individual request level to the carousel.

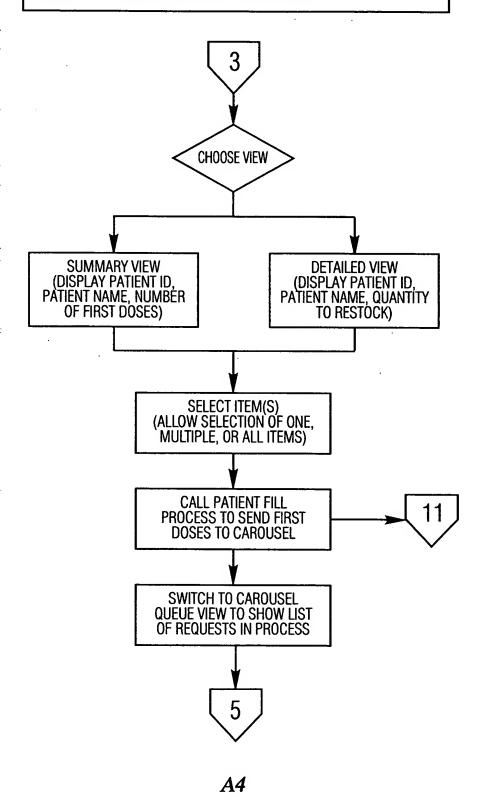



Defines the patient cart filling process. This allows the viewing of queued cart fill dispenses and the ability to selectively send these requests on a delivery unit or patient level to the carousel.

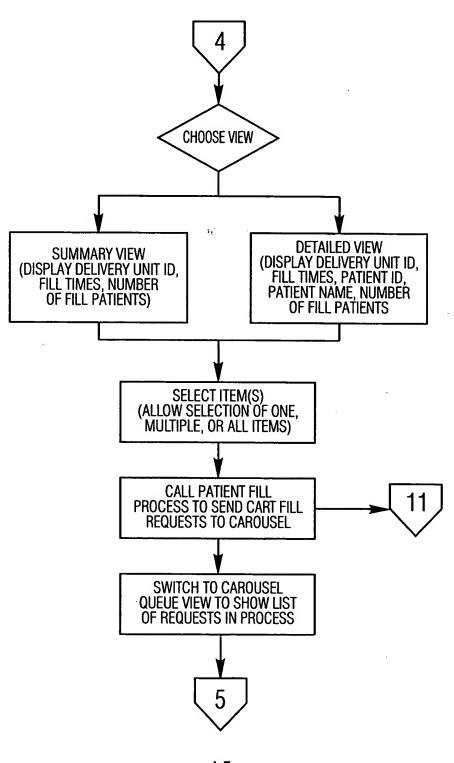


Defines the processing flow of the carousel queue screen. This screen displays the requests that have been sent to the carousel, including the request currently being processed and the requests that are waiting behind the current request. In auto-mode, the carousel will automatically move to the next request.

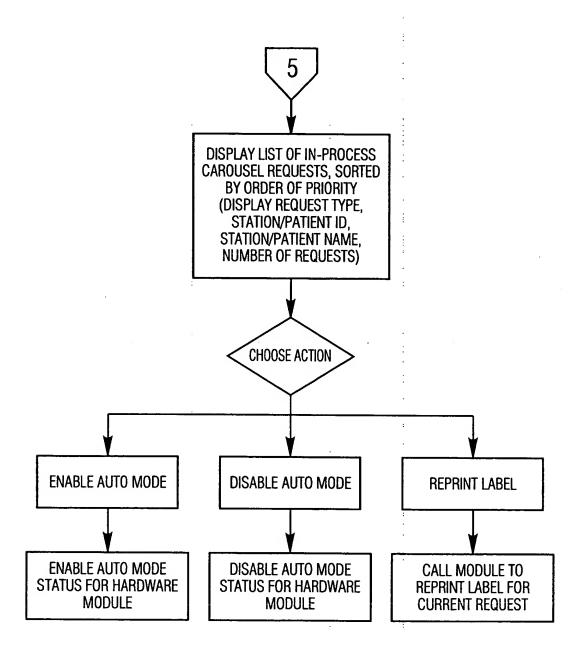

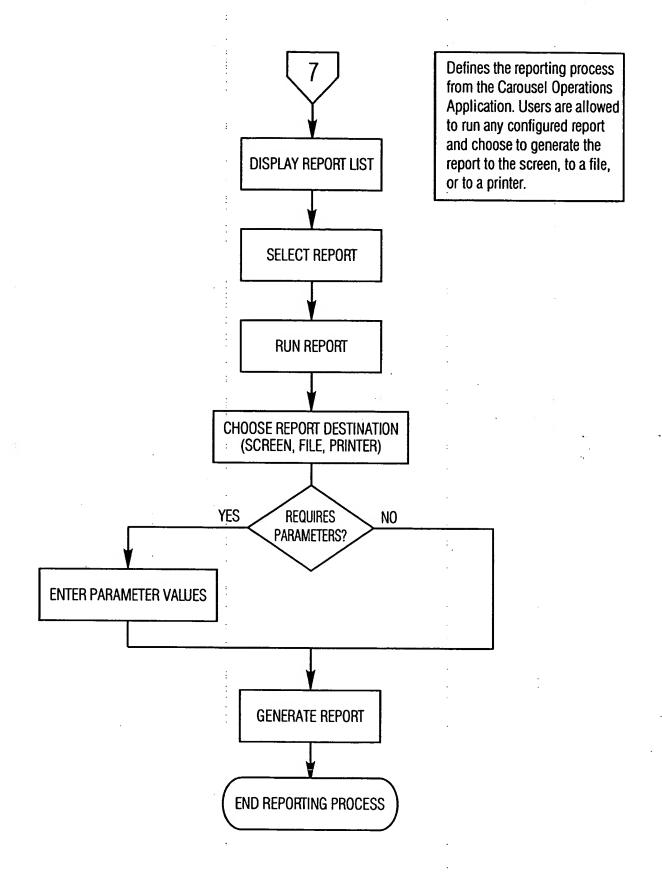

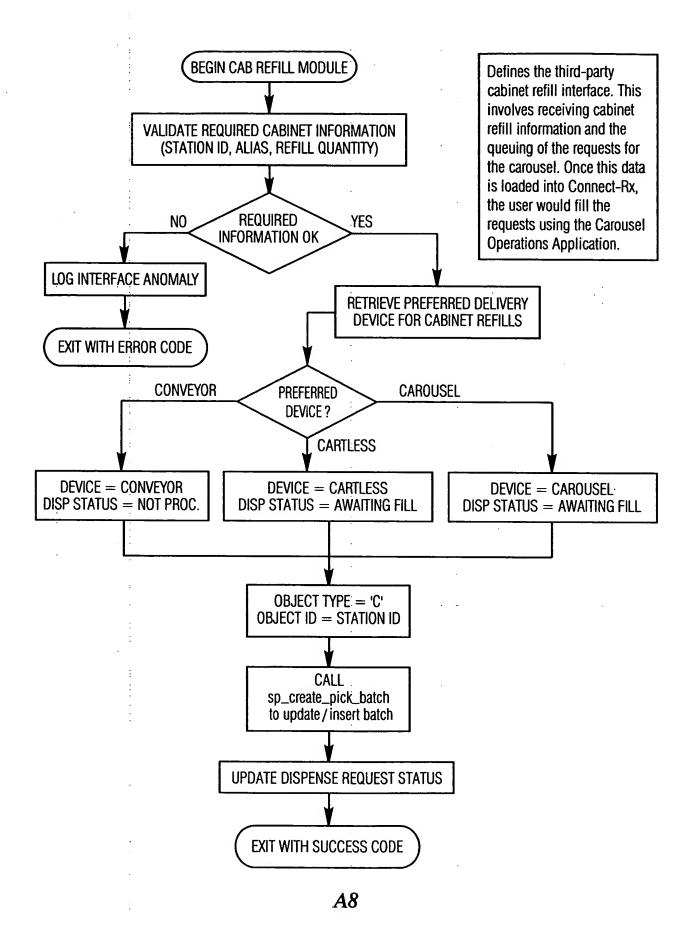

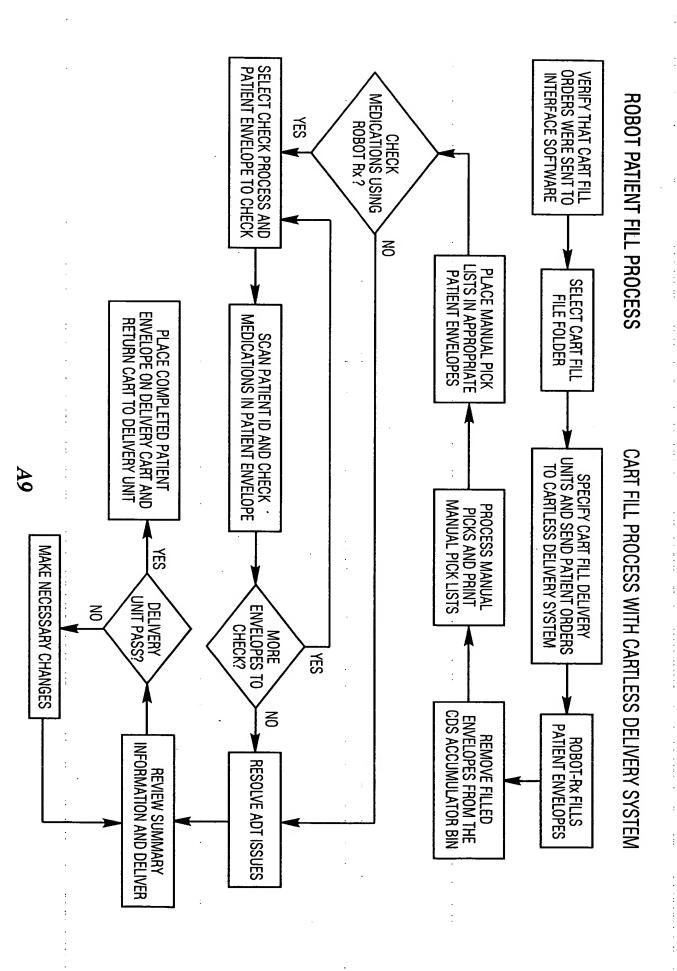

ROBOT CABINET FILL PROCESS

CABINET RESTOCKING PROCESS

